

# Failed Calibration Summary (All Companies)


By Company  
Calibrations from 10/10/2000 to 12/12/2016

## Quality Lab Inc

### List of As Left and As Found Failures

ID #:	Item Type:	CalibrationDate	Item Name:	Manufacturer:	Department:	Location:
32	Instrument	6-Aug-2010	Sample Balance	Sartorius	Lab	Laboratory
10	Instrument	18-Apr-2006	pH Indicator / ASH Pit	YOKOGAWA		Process Plant
12	Instrument	20-Dec-2007	Caliper	Mitutoyo	Production	Process Plant
35	Instrument	10-Aug-2010	Water Conductivity	Thorton	Facilities	QLI West Chester, PA
34	Instrument	6-Aug-2010	Sample Balance	Sartorius	Lab	Laboratory
1	Instrument	17-May-2016	Temperature Indicator			QLI West Chester, PA

### Failed Calibration Summary (Quality Lab Inc)

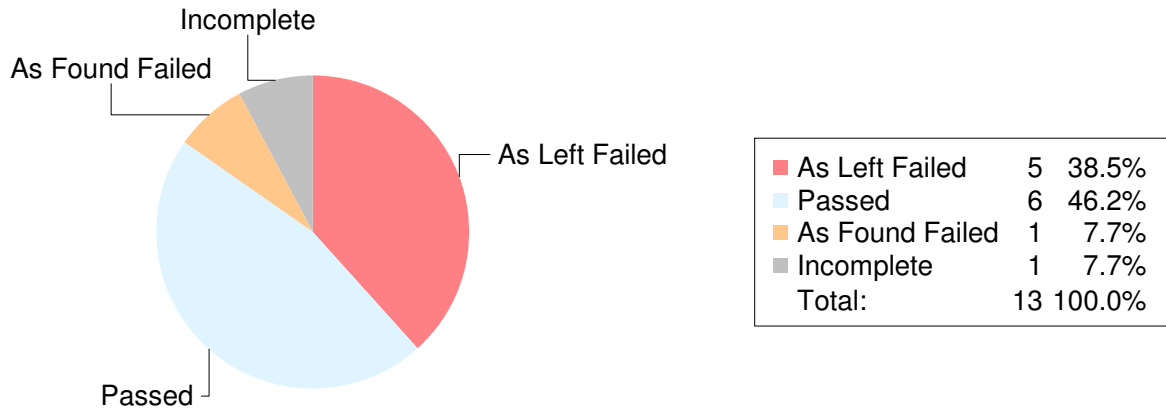


## Template Company

### List of As Left and As Found Failures

ID #:	Item Type:	CalibrationDate	Item Name:	Manufacturer:	Department:	Location:
29	Instrument	6-Aug-2010	Admin Utility Test Instr 1	Rosemount - 1151	Template Metrology Dept	
31	Instrument	6-Aug-2010	Blank General Info Tab fields	Rosemount - 1151		
30	Instrument	6-Aug-2016	Admin Utility Test Instr 1	Rosemount - 1151	Template Metrology Dept	

## Failed Calibration Summary (Template Company)

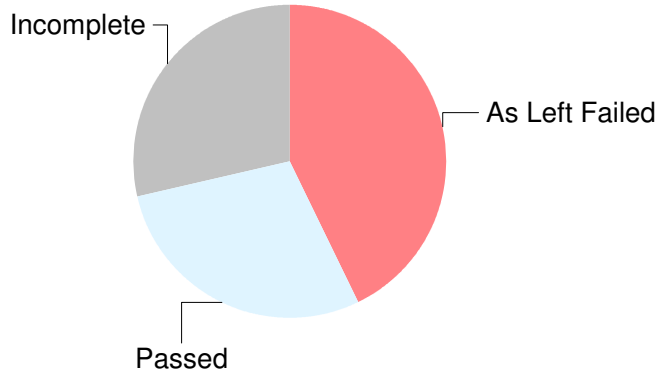


As Left Failed	3	42.9%
Passed	2	28.6%
As Found Failed	0	0.0%
Incomplete	2	28.6%
<b>Total:</b>	<b>7</b>	<b>100.0%</b>

## Validation Management

### List of As Left and As Found Failures

ID #:	Item Type:	CalibrationDate	Item Name:	Manufacturer:	Department:	Location:
25	System	5-Oct-2009	G Lab - Thermo/IEC GP8K Centrifuge	Thermo/IEC	Vaccines	West Chester

## Failed Calibration Summary (Validation Management)

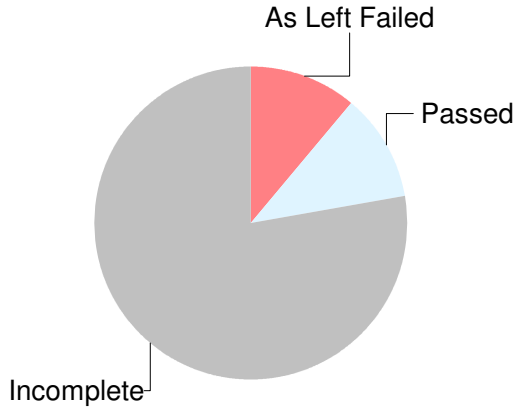

As Left Failed	1	11.1%
Passed	1	11.1%
As Found Failed	0	0.0%
Incomplete	7	77.8%
<b>Total:</b>	<b>9</b>	<b>100.0%</b>

# All Failures by Company

